Pacifier clinical thermometer
Geratherm© daisy color GT-126

Geratherm Medical AG
Germany

GB

Please read carefully before using.

FEATURES

1. With visual fever alarm.
2. Baby pacifier with orthodontic nipple design, made of hard-wearing silicon.
3. Easy-to-read large LCD (liquid crystal display).
4. The device is waterproof.
5. No mercury inside.

PARTS DESCRIPTION

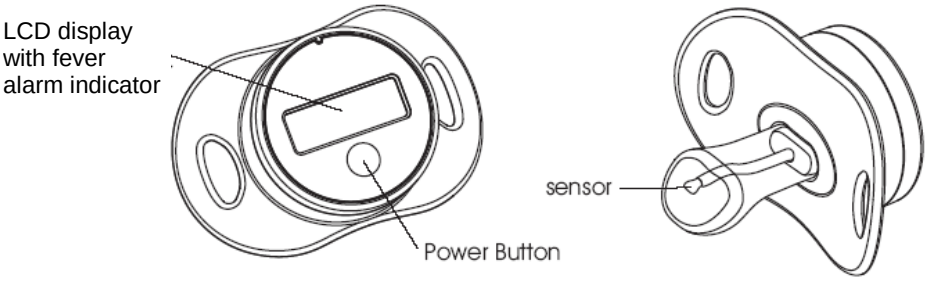

SPECIFICATIONS

Range:	32.0~43.9°C; below 32.0°C, display L°C; above 43.9°C, display H°C
Resolution:	0.1°C
Accuracy:	±0.1°C (34.0°C to 42.0°C), ±0.2°C (other ranges)
Display:	Liquid crystal display 3 1/2 digits
Battery (included):	CR2032 (3V)
Power consumption:	0.15 milliwatts in measurement mode
Battery life:	More than 160 hours of continuous operation
Dimensions:	60mm x 50mm x 42mm
Weight:	Approx. 23 grams (including battery)
Beeper:	Approx. 3 secs. sound signal when end temperature reached
Memory:	Built-in memory enabling display of the previously measured value
Shut-off:	Automatic shut-off in approx. 30 seconds
Operating conditions:	Temperature: 10°C~40°C; Humidity: 15%~95% non condensing
Storage conditions:	Temperature: -20°C~60°C; Humidity: 15%~95% non condensing
Guarantee of quality:	Certification acc. to ISO 13485 and 93/42/ EEC, Annex II; thermometer conforms to EN 12470-3:2000 (Medical Thermometers, Part 3: Performance of compact electrical (extrapolating and non-extrapolating) thermometers with maximum device) excepted 6.2.4 (response time), EN60601-1
Product classification:	Type BF

BATTERY DISPOSAL

For safety reasons, the battery cannot be exchanged.

1. When the symbol " " appears, the unit should be disposed of. Discard the battery before disposing of the unit.
2. Separate the panel sticker from the unit.
3. Use a screwdriver to do it.
4. Discard the battery.

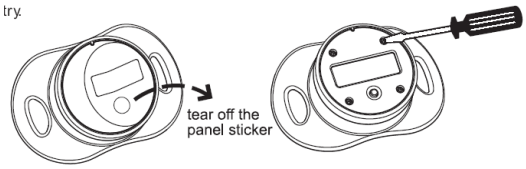

Warning: Keep the thermometer and battery out of reach of young children. If the battery is swallowed, contact a hospital immediately to have it removed. Do not dispose of the battery in a fire. It may explode.

PRECAUTIONS

- Before every use, check the pacifier thermometer and especially the silicon nipple for signs of damage or wear.
- Do not use damaged pacifier any more.
- Always maintain the minimum time required for measurement which is indicated by the acoustic signal.
- The pacifier thermometer is intended only for oral measurement of body temperature in children up to 3 years of age.

- It is not suitable for constant sucking.
- Under specific conditions (crying, breathing through the mouth), the displayed temperature may be too low.
- In case of doubt and signs of fever (temperature higher than 38.5°C, flushed appearance, perspiration, unwillingness to drink, restlessness) measure the body temperature rectally.
- Keep out of reach of unsupervised children.
- Do not drop the thermometer or expose it to heavy shock.
- Do not boil the probe.
- Do not store the unit under direct sunlight, at a high temperature, or in high humidity or dust. Performance may be degraded.
- Do not try to take the thermometer apart.
- Observe the applicable regulations when discarding the device and the batteries.

HOW TO USE

1. Remove the protective cover.
2. Place the pacifier nipple in the child´s mouth like a normal baby pacifier. Be sure the child keeps the thermometer in his mouth during measurement, and keep the child´s mouth closed as much as possible.
   Note: Drinking or eating prior to use may affect the reading.
3. Start with the measurement after abt. 3 – 5 minutes by pressing the ON/OFF button. The display will read with fever alarm indicator flashing (red -> yellow -> green) for 2 seconds.
4. The display will show L,°C with °C flashing.
5. Once the degree sign °C stops flashing, the measurement is ready and the correct temperature is displayed. An alarm will sound for approximately 3 seconds after measurement.
6. The fever alarm indicator (colored backlight) will light up for 5 seconds, the color depending on the temperature measured. It is recommended to leave the thermometer in the baby`s mouth to allow the nipple to warm up and obtain a more accurate reading.
7. The unit will automatically turn off in approx. 30 seconds. However, to save energy, it is best to turn the thermometer off immediately after the temperature has been noted.

Note: Oral temperature readings are often 0.5°C lower than actual body temperature readings.

Special Features:
Last-temperature memory recall:
Press and hold the ON/OFF button while turning on the unit for more than 3 seconds. The last measured temperature will appear with the letter “M” under the °C sign.

Visual fever alarm: If the temperature registers higher than 37.5 °C, the display will have a red background light for 5 seconds.

temperature	**fever alarm indicator**
36.0 ≦ T ≦ 37.1	**green**
37.2 ≦ T ≦ 37.4	**yellow**
37.5 ≦ T ≦ 43.9	**red**

NOTE: Children should be attended by an adult during the entire temperature recording process. After use, the digital pacifier thermometer should be stored in a safe place, out of reach of young children.

CLEANING INSTRUCTIONS

Disinfect the thermometer by wiping the teat (with the sensor) and the shield with a cloth that has been immersed in a household antiseptic solution, such as rubbing alcohol.

LIMITED WARRANTY

This thermometer is guaranteed for 2 years from the date of purchase against manufacturer’s defect under normal use. The warranty does not cover damage to your unit due to improper handling. Following the directions closely will ensure years of dependable operation.
In case of professional use, the manufacturer recommends to verify the accuracy by an authorized laboratory every 2 years (in Germany this is compulsory).

Manufacturer:
Geratherm Medical AG
Fahrenheitstraße 1
D-98716 Geschwenda
Germany

CE 0118